



# Co2 Adjustment - Plus RA

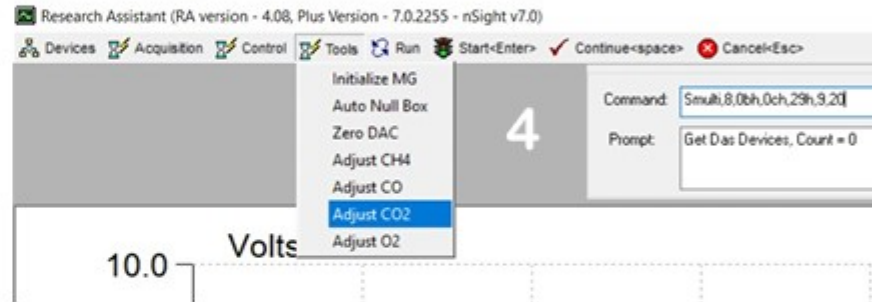

With the case removed from the GEM, adjust the Co2 control until  
 The Difference is as close as you can achieve to 3.3v ( + - 0.05v )  
 Now come out of Plus RA, go into the KoKo software, and perform the  
 normal Co2 / MGA Calibrations.

	Channel ID	Channel Name	Current	Min	Max	Diff	Average
Channel 1	12 (Ch)	He1, GMCO2				<b>3.3</b>	

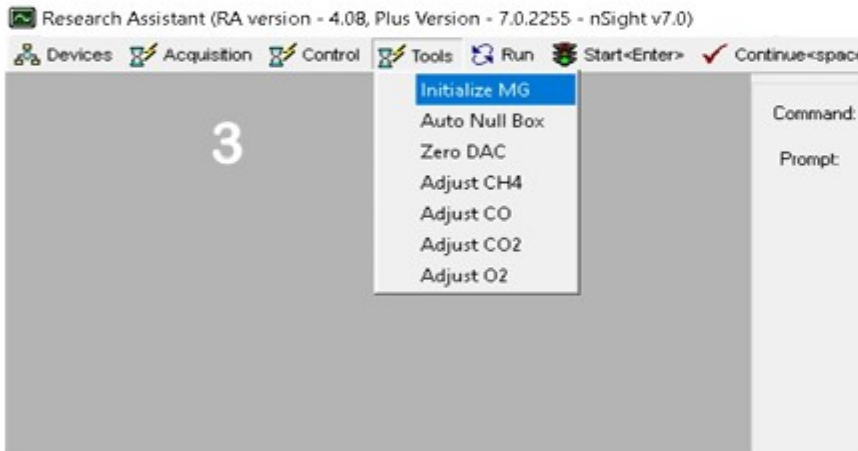